

n-trapped arg lamp




Current Data Parameters
NAME Nov29-2017
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date 20171129
Time 12.57
INSTRUM spect
PROBHD 5 mm BBO BB-1H
PULPROG zg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8250.825 Hz
FIDRES 0.125898 Hz
AQ 3.9715922 sec
RG 1149.4
DW 60.600 usec
DE 6.00 usec
TE 0.0 K
D1 1.00000000 sec
MCREST 0.00000000 sec
MCWRK 0.01500000 sec

===== CHANNEL f1 =====
NUC1 1H
P1 10.00 usec
PL1 0.00 dB
SFO1 400.1324710 MHz

F2 - Processing parameters
SI 32768
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

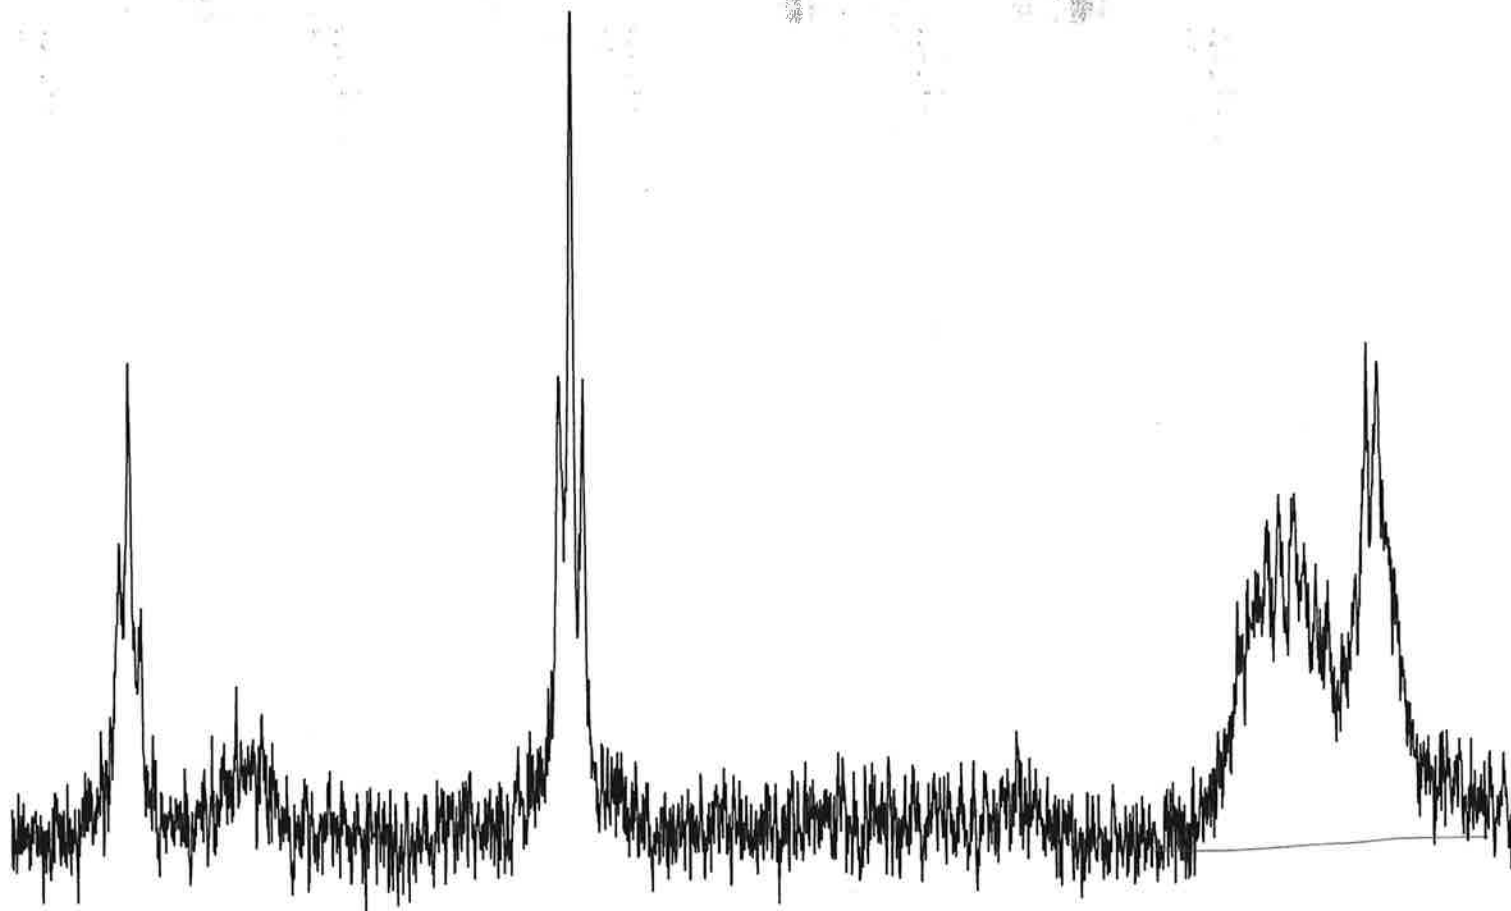

2.6 2.5 2.4 2.3 2.2 2.1 2.0 1.9 1.8 1.7 1.6 1.5 1.4 1.3 1.2 1.1 1.0 0.9 0.8 0.7 ppm

1.35