



Device 1

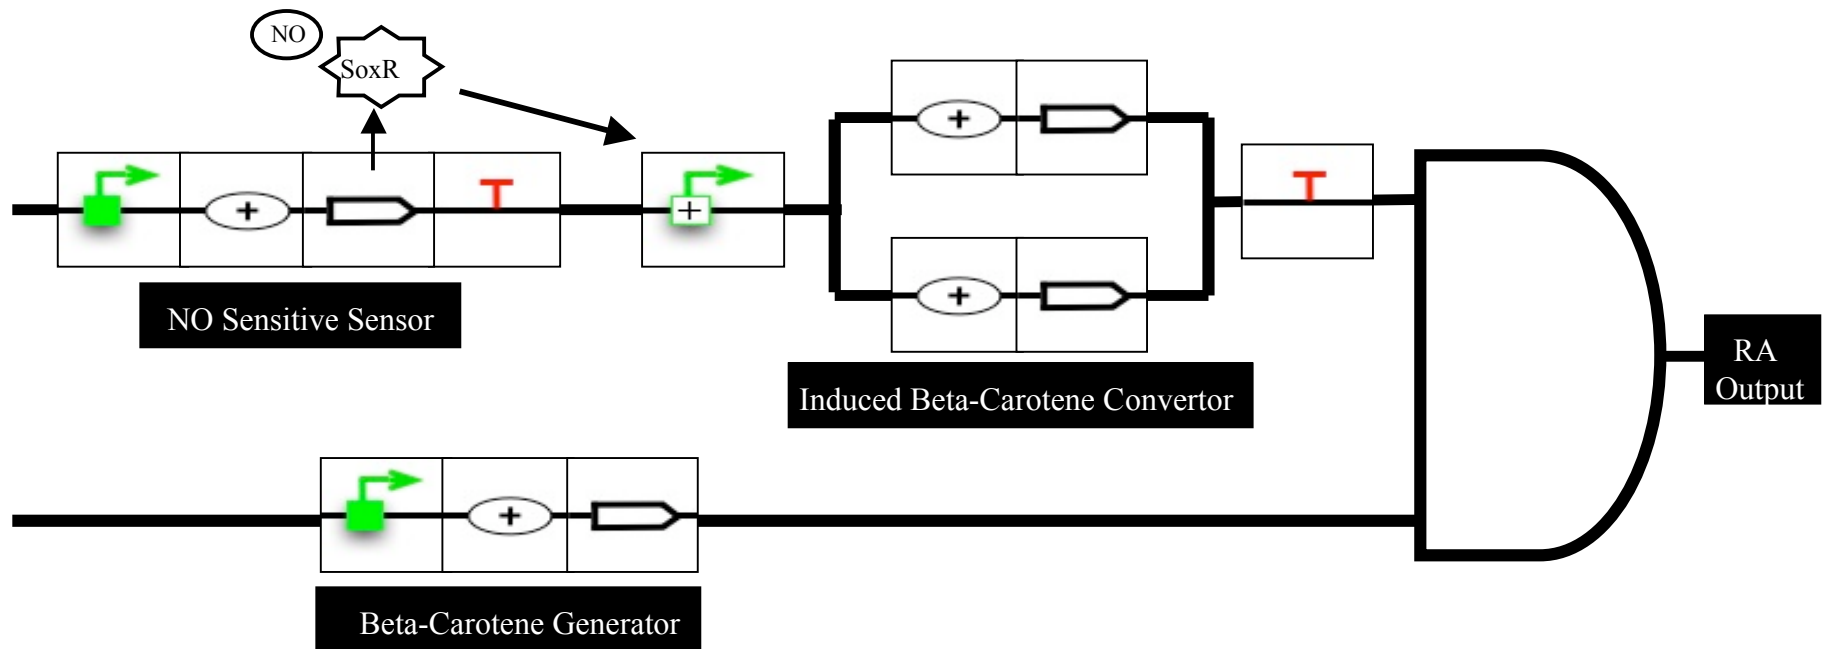


Device 1

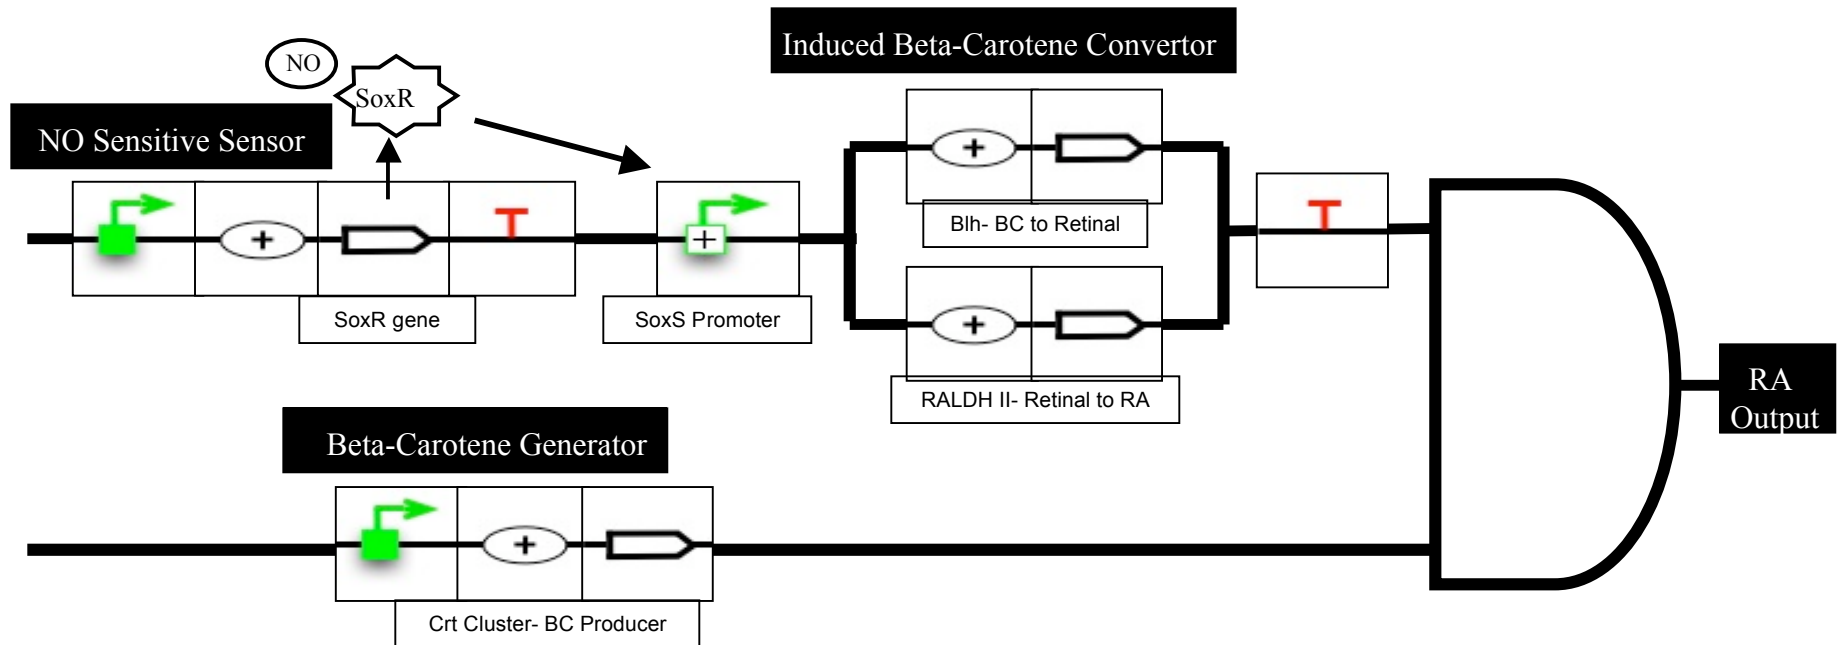


Device 1


Induced Beta-Carotene Converter

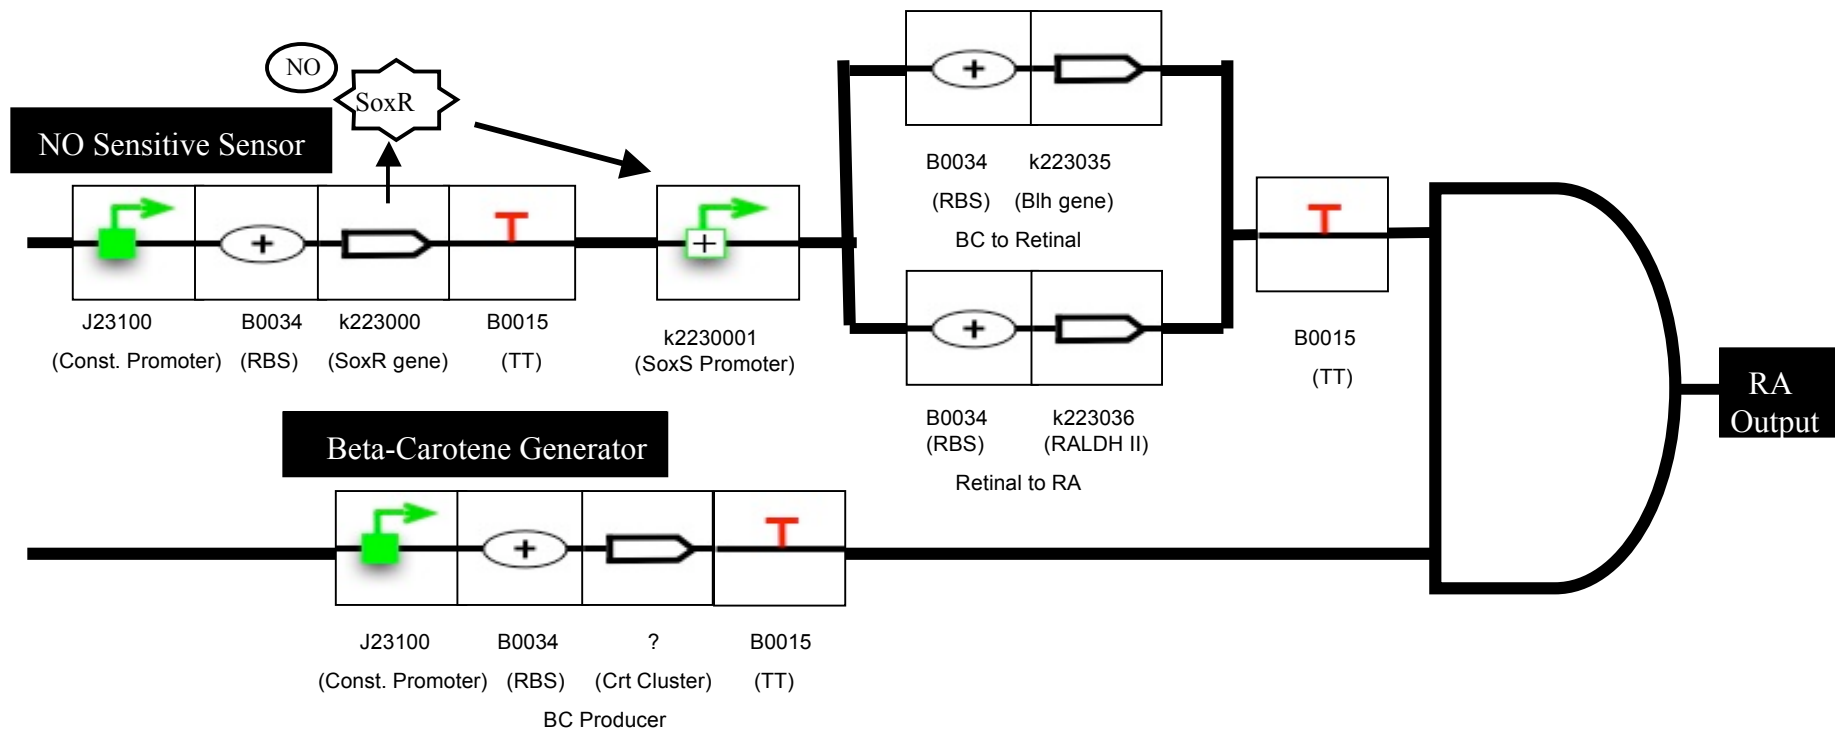

Device 2

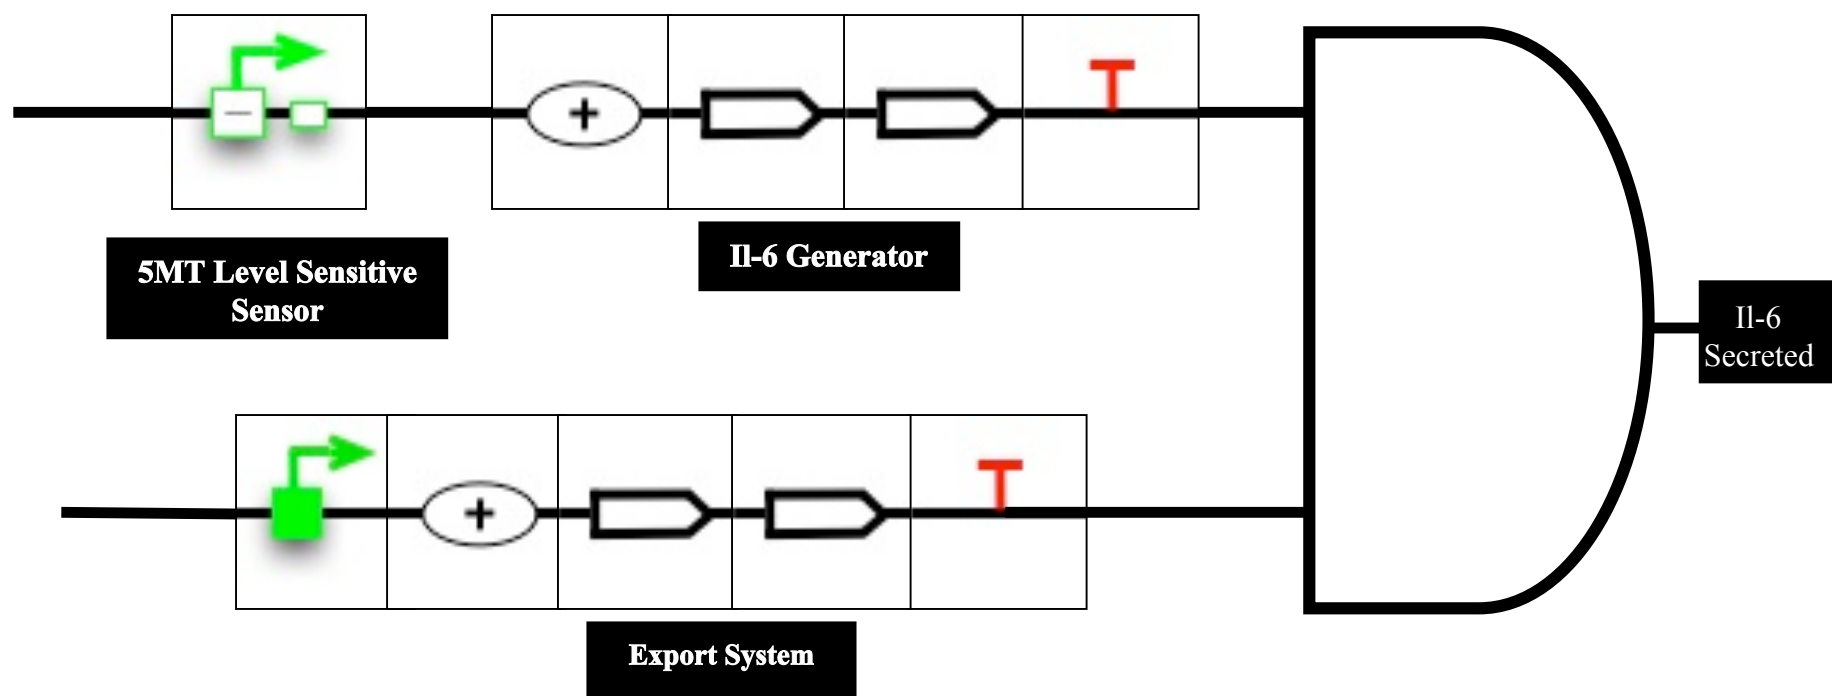


Device 2

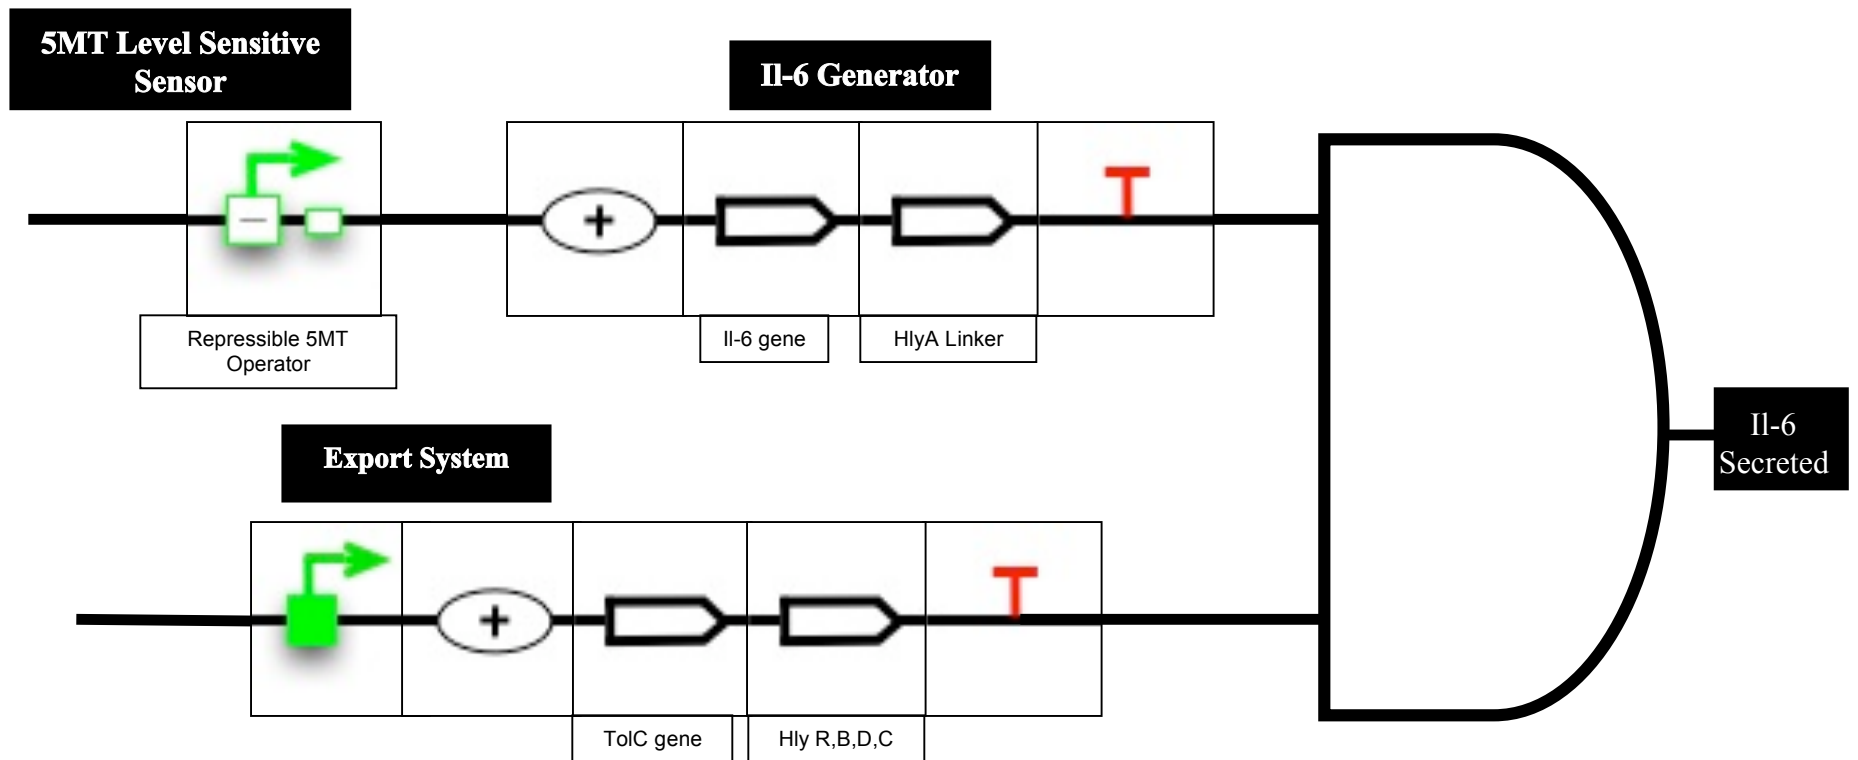

Device 2

5MT Level Sensitive Sensor

Il-6 Generator

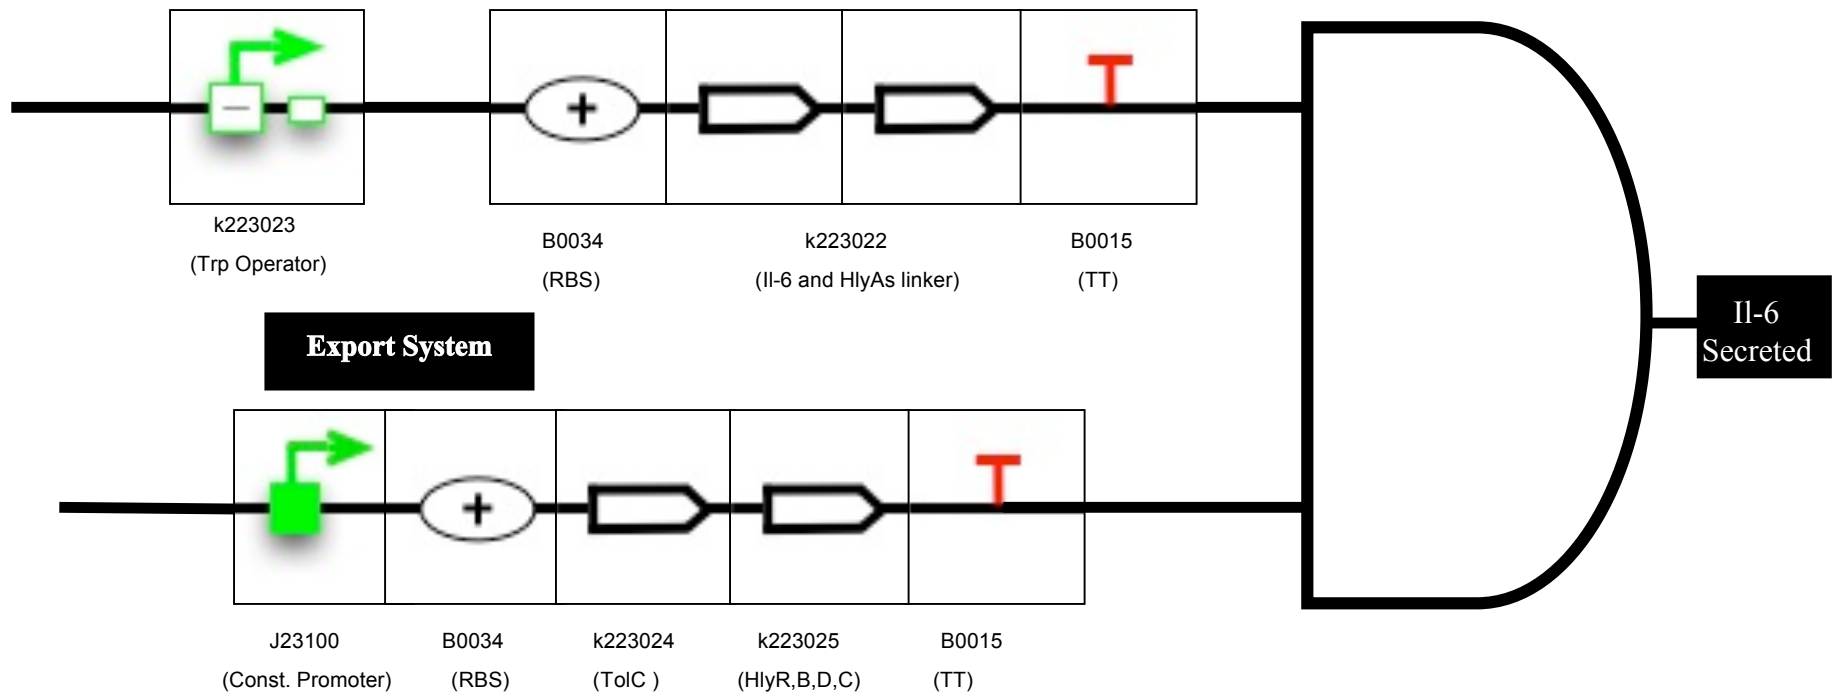

Device 1

