


Bromophenol - pH: 6

SmartSpec (TM) Plus Report  
09:46 11/17/11  
Operator: amira  
Scan Report

start wavelength: 400 nm  
end wavelength : 700 nm

max: 588 : 1.019 AU  
min: 689 : -0.037 AU

0.000 2.000

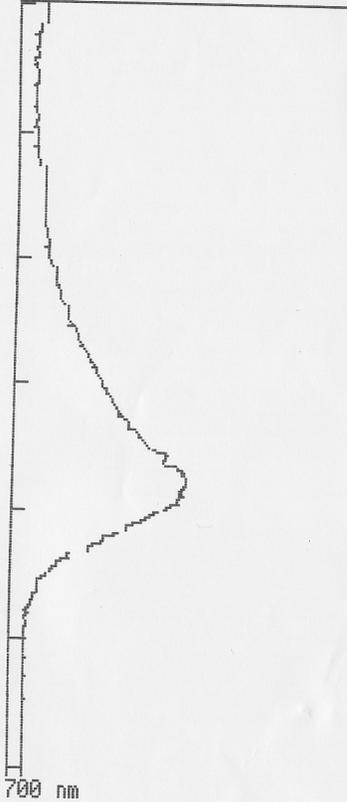

x axis: 50 nm/division

20x x 11/17/11


pH: 5.5

SmartSpec (TM) Plus Report  
10:12 11/17/11  
Operator: amira  
Scan Report

start wavelength: 400 nm  
end wavelength : 700 nm

max: 439 : 0.704 AU  
min: 697 : -0.021 AU

0.000 1.000

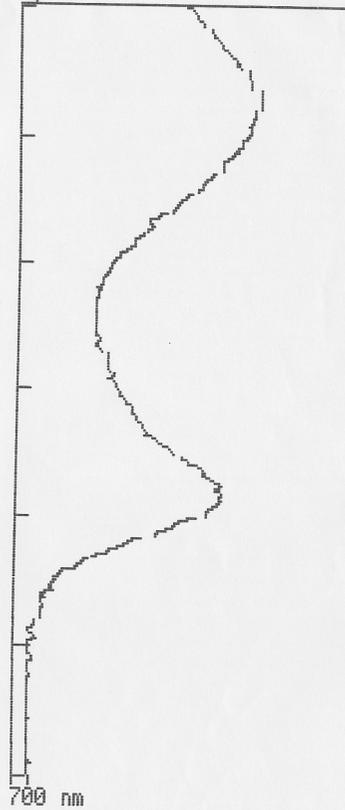

x axis: 50 nm/division


pH 4.5

SmartSpec (TM) Plus Report  
09:51 11/17/11  
Operator: amira  
Scan Report

start wavelength: 400 nm  
end wavelength : 700 nm

max: 434 : 0.859 AU  
min: 688 : -0.013 AU

0.000 1.000

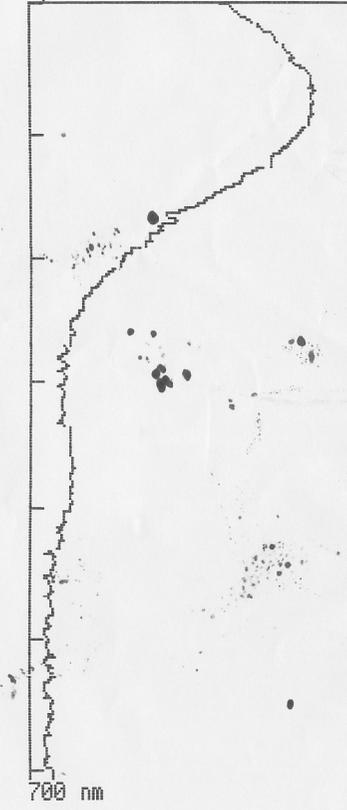

x axis: 50 nm/division


pH: 3

SmartSpec (TM) Plus Report  
09:53 11/17/11  
Operator: amira  
Scan Report

start wavelength: 400 nm  
end wavelength : 700 nm

max: 433 : 0.866 AU  
min: 688 : -0.030 AU

0.000 1.000

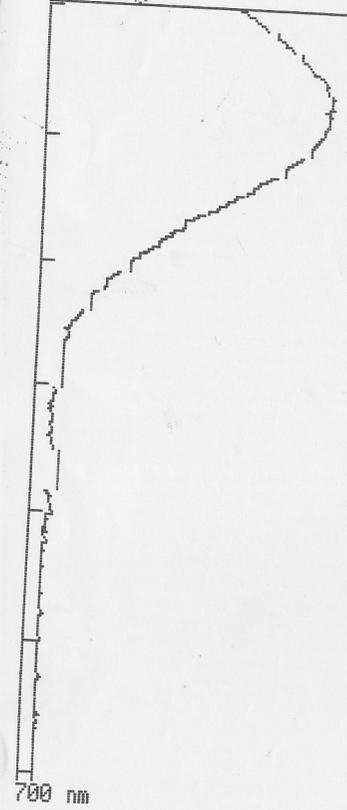

x axis: 50 nm/division